







Test Report SL52035260354401TX Date: June 28,2020 Page 1 of 6

DONGGUAN MAYNALUCY FOOTWEAR CO., LTD ROOM 101 NO.1, JINSHUN HENG ROAD, HOU JIE TOWN, DONG GUAN CITY, GUANGDONG, CHINA

The following sample(s) was/were submitted and identified on behalf of the client as:

Sample Description : (A)DISPOSABLE FACE MASK

Style No. : Skylar DGMC-001

Composition : (A)60%Non-Woven 40%Melt-Blown Fabric

Sample Color : (A)White

Manufacturer : DONGGUAN MAYNALUCY FOOTWEAR CO., LTD

Country of Destination : Europe

Supplier : MAYNALUCY

Previous Report No. : SL52035260369001TX

Test Performed : Selected test(s) as requested by applicant

Sample Receiving Date : Jun 12, 2020

Testing Period : Jun 16, 2020 - Jun 28, 2020

Test Result(s) : Unless otherwise stated the results shown in this test report refer only to the

sample(s) tested, for further details, please refer to the following page(s).

Based on the results of the tests reported and the previous report SL52035260369001TX issued on Jun 16,2020, our Lab concluded that the recommendation level can be as below.

Sample No.	Recommendation Level
(A)	FFP2 NR

Signed for and on behalf of SGS-CSTC Standards Technical Services (Shanghai) Co., Ltd Testing Center



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com/en/Terms-and-Conditions.apx and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@cgs.com

Sara Guo (Account Executive)

Test Result

<u>Personal Protective Equipment - Respiratory Protective Devices- Filtering Half Masks to Protect against Particles- Requirements, Testing, Marking</u>

EN 149:2001+A1:2009

Clause 7.4 Packaging

(EN 149:2001+A1:2009 Clause 8.2)

Test Requirement	Results	Comment
Particle filtering half masks shall be offered for sale packaged in such a way that they are protected against mechanical damage and contamination before use.	Comply	Pass

Clause 7.7 Practical Performance

(EN 149:2001+A1:2009, Clause 8.4)

Test Requirement	Results	Comment
The particle filtering half mask shall undergo practical performance tests under realistic conditions. These general tests serve the purpose of checking the equipment for imperfections that cannot be determined by the tests described elsewhere in this standard.	No imperfections	Pass

Clause 7.8 Finish of Parts

(EN 149:2001+A1:2009, Clause 8.2)

Test Requirement	Results	Comment
Parts of the device likely to come into contact with the wearer shall have no sharp edges or burrs.	No sharp edges or burrs	Pass

Clause 7.9.1 Total Inward Leakage

(EN 149:2001+A1:2009, Clause 8.5)

Re	Test Requirement Results	Comment
----	--------------------------	---------



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com/en/Terms-and-Conditions/Terms

3rdBuilding,No.889,Yishan Road,Xuhui District Shanghai,China 200233 中国・上海・徐汇区宜山路889号3号楼 邮编: 200233 t (86-21) 61402666 t (86-21) 61402666 f (86-21) 64958763 f (86-21) 64958763

Test Report

Date: June 28,2020



The total inward leakage consists of three components: face seal leakage, exhalation value leakage(if exhalation value fitted) and filter penetration. For particle filtering half masks fitted in accordance with the manufacturer's information, at least 46 out of the 50 individual exercise results (i.e. 10 subjects x 5 exercises) for total inward leakage shall be not greater than: 25% for FFP1, 11% for FFP2, 5% for FFP3	Detail refer to Appendix 1	Meet FFP1 Meet FFP2
and, in addition, at least 8 out of the 10 individual wearer arithmetic means for the total inward leakage shall be not greater than: 22% for FFP1, 8% for FFP2, 2% for FFP3		

Appendix 1: Summarization of Test Data

Inward Leakage Test Data

iniviara Ed	akage rest	<u> </u>			-		1	
Subject	Sample No.	Condition	Walk(%)	Head Side/side(%)	Head up/down(%)	Talk(%)	Walk(%)	Mean(%)
				0.00/0.00(70)	ap/aom.(70)			
Zhou	1	A.R.	5.77	6.92	5.84	5.75	6.47	6.15
Luo	2	A.R.	7.66	7.20	6.27	8.11	6.74	7.08
Lu	3	A.R.	4.92	6.23	6.23	7.32	5.77	6.09
Wang	4	A.R.	4.38	5.07	4.76	5.04	5.76	5.00
Bao	5	A.R.	6.62	8.48	7.09	6.83	6.94	7.07
Ding	6	T.C.	4.45	5.00	6.15	5.79	4.41	5.16
Li	7	T.C.	8.26	7.25	7.42	6.83	6.35	7.22
Chen	8	T.C.	5.63	5.14	4.78	5.99	5.21	5.35
Song	9	T.C.	6.26	6.34	7.36	5.40	7.62	6.60
Ye	10	T.C.	6.42	7.41	7.85	7.39	7.21	7.26

Facial Dimension(mm)

Subject	Face length	Face Width	Face Depth	Mouth Width
Chen	125	150	120	58
Lu	115	132	107	48
Zhou	115	135	106	52
Li	125	130	107	46
Luo	125	136	100	43
Zheng	128	140	112	55
Wang	120	147	103	48
Song	120	140	100	50
Bao	130	134	104	50
Ding	134	150	110	52
Liu	120	135	117	50
Ye	126	137	105	52



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com/en/Terms-and-Conditions.aspx and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com/en/Terms-and-Conditions/Terms-and-Cond

3rdBuilding, No. 889, Yishan Road, Xuhui District Shanghai, China 200233 中国・上海・徐汇区宜山路889号3号楼 邮编: 200233 t (86-21) 61402666 t (86-21) 61402666 f (86-21) 64958763 f (86-21) 64958763



Clause 7.13 Head Harness

(EN 149:2001+A1:2009, Clause 8.4 & 8.5)

Test Requirement	Results	Comment
The head harness shall be designed so that the particle filtering half mask can be donned and removed easily.	Comply	
The head harness shall be adjustable or self-adjusting and shall be		Pass
sufficiently robust to hold the particle filtering half mask firmly in position and be capable of maintaining total inward leakage requirements for the device.	Comply	

Clause 7.14 Field of Vision

(EN 149:2001+A1:2009, Clause 8.4)

Test Requirement	Results	Comment
The field of vision is acceptable if determined so in practical performance tests.	Comply	Pass

Clause 7.18 Demountable Parts

(EN 149:2001+A1:2009, Clause 8.2)

Test Requirement	Results	Comment
All demountable parts (if fitted) shall be readily connected and secured, where possible by hand	No demountable parts	N.A.

Test	Uncertainty
Total inward leakage	3.4%
Penetration of filter material	4.8%
Carbon dioxide content of the inhalation air	3.9%
Breathing resistance (30L/min)	5.9%
Breathing resistance (95L/min)	4.9%
Breathing resistance (160L/min)	4.3%

Sample Photo




Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com/en/Terms-and-Conditions/Terms

3rdBuilding,No.889,Yishan Road,Xuhui District Shanghai,China 200233 中国・上海・徐汇区宜山路889号3号楼 邮编: 200233 t (86-21) 61402666 t (86-21) 61402666 f (86-21) 64958763 f (86-21) 64958763

Test Report

SL52035260354401TX

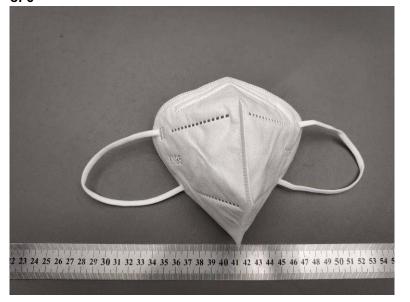






Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com/en/Terms-and-Conditions.aspx and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Document.aspx. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 83071443, or email: CN.Doccheck@cgs.com

3rdBuilding,No.889,Yishan Road,Xuhui District Shanghai,China 200233 中国・上海・徐汇区宜山路889号3号楼 邮编: 200233 t (86-21) 61402666 t (86-21) 61402666 f (86-21) 64958763 f (86-21) 64958763

Test Report of 6







End of Report



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at http://www.sgs.com/en/Terms-and-Conditions.aspx and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <a href="http://www.sgs.com/en/Terms-and-Conditions/Terms-and-Cond

3rdBuilding,No.889,Yishan Road,Xuhui District Shanghai,China 200233 中国・上海・徐汇区宜山路889号3号楼 邮编: 200233 t (86-21) 61402666 t (86-21) 61402666

f (86-21) 64958763 f (86-21) 64958763